


- | | |
|-----------------------|-------------------|
| 1. Desethylatrazine | 10. Diuron |
| 2. Metoxuron | 11. Isoproturon |
| 3. Hexazinone | 12. Metobromuron |
| 4. Simazine | 13. Metazachlor |
| 5. Cyanazine | 14. Sebuthylazine |
| 6. Methabenzthiazuron | 15. Terbutylazine |
| 7. Chlorotoluron | 16. Linuron |
| 8. Atrazine | 17. Metolachlor |
| 9. Monolinuron | |

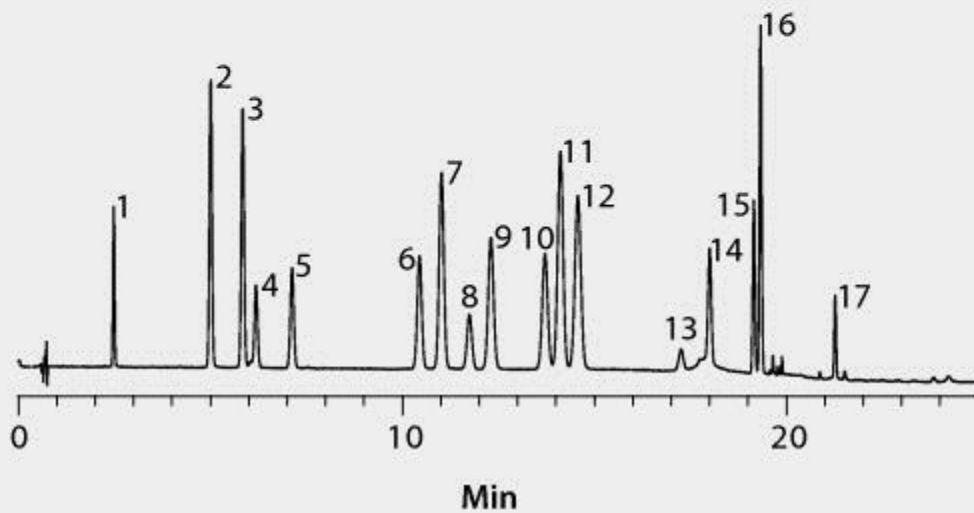

test parameters	column: Ascentis Express C18, 10 cm x 3.0 mm I.D., 2.7 µm particles (53814-U)
	mobile phase: (A) 20 mM ammonium acetate, pH 6.4 unadjusted; (B) acetonitrile
	gradient: 20 to 28% B in 11 min; 28 to 65% B in 5 min; held at 65% B for 4 min
	flow rate: 0.6 mL/min
	column temp.: 46 °C
	detector: UV, 240 nm
	injection: 5 µL