


1. Thyroglobulin, 669,000 Da
2. Ferritin, 440,000 Da
3. Albumin, 66,000 Da
4. Carbonic anhydrase, 29,000 Da
5. Aprotinin, 6,500 Da
6. p-Aminobenzoic acid, 137 Da

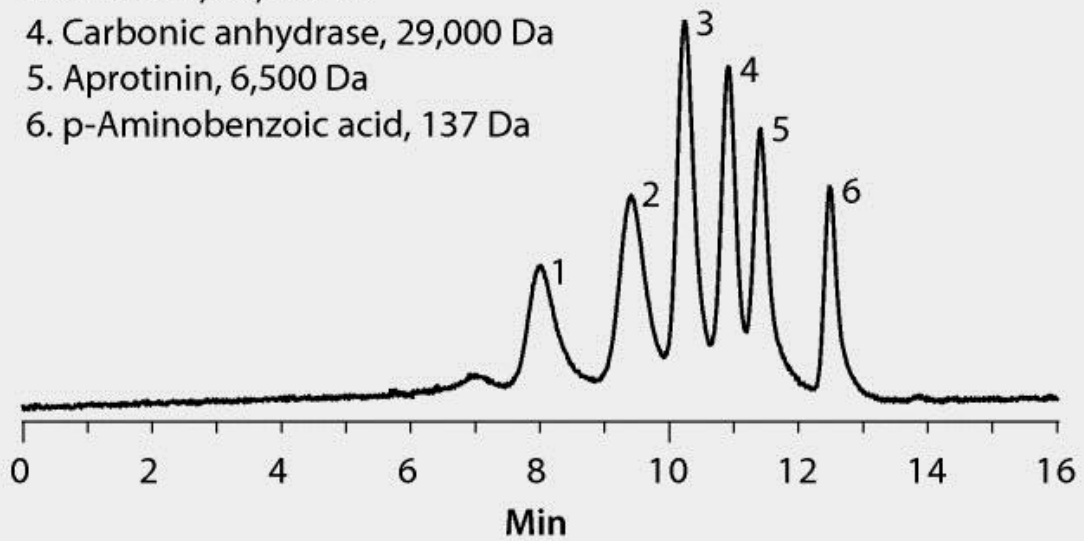

test parameters	column: Discovery BIO GFC 500, 30 cm x 7.8 mm I.D., 5 µm particles (567308-U)
	mobile phase: 150 mM potassium phosphate monobasic, pH 7.0
	flow rate: 1.0 mL/min
	column temp.: 25 °C
	detector: UV, 280 nm
	injection: 10 µL
	sample: 1-10 g/L in buffer