


1. Thyroglobulin, 669,000 Da
2.  $\gamma$ -Globulins, ~300,000 Da
3. Ovalbumin, 44,281 Da
4. Myoglobin, 17,699 Da
5. Poly-DL-alanine, 1,000-5,000 Da
6. Uracil, 112 Da

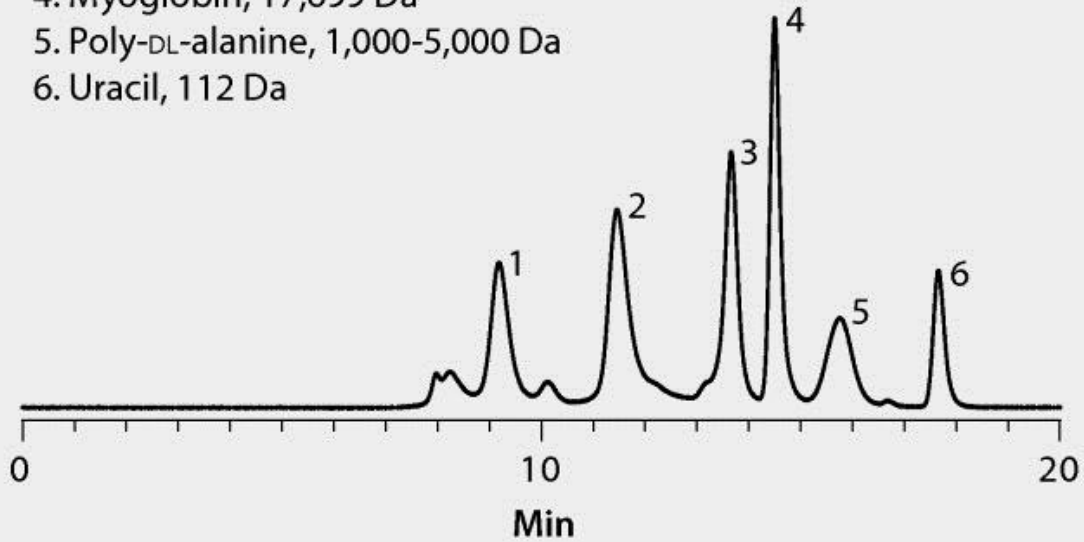

test parameters	<p>column: Discovery BIO GFC 300, 30 cm x 4.6 mm I.D., 3 <math>\mu</math>m particles (567335-U)</p> <p>mobile phase: 150 mM potassium phosphate monobasic, pH 7.0 (adjusted with potassium hydroxide)</p> <p>flow rate: 0.25 mL/min</p>
	pressure: 45 bar
	column temp.: 25 $^{\circ}$ C
	detector: UV, 214 nm
	injection: 1 $\mu$ L
	sample: 1 g/L each (except uracil, 0.1 g/L) in mobile phase