


1. Threonine (0.1 g/L)
2. Serine (0.1 g/L)
3. Asparagine (0.1 g/L)
4. Glutamine (0.1 g/L)
5. Glutamic acid (0.1 g/L)
6. Aspartatic acid (0.1 g/L)

Gradient Program			
Time (min)	%A	%B	%C
0	5	10	85
20	5	16	79

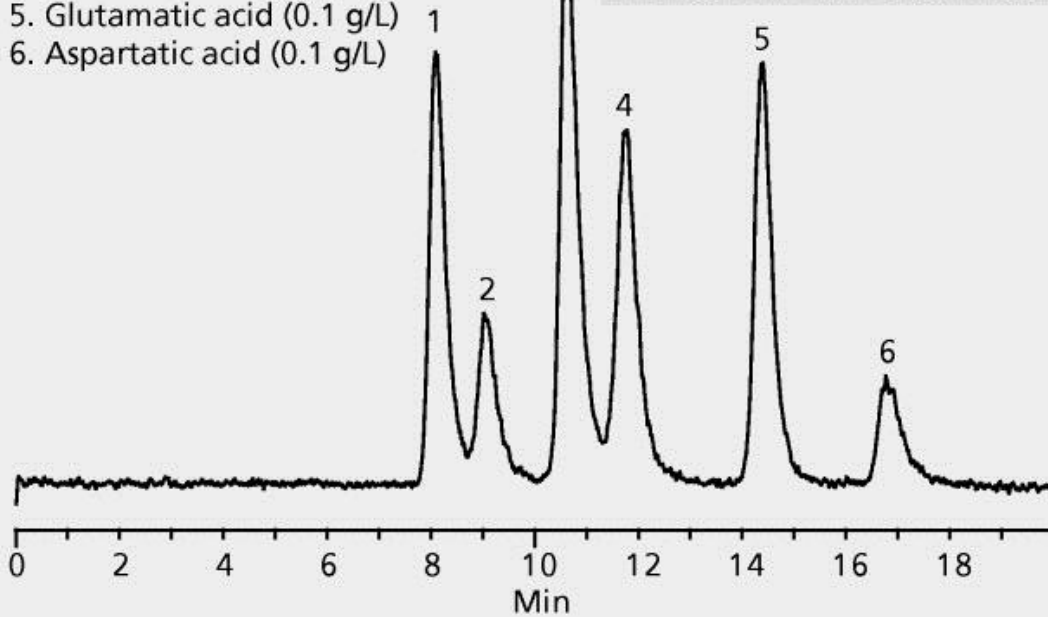

test parameters	column: Ascentis Si, 10 cm x 2.1 mm I.D., 5 μ m particles (581508-U)
	mobile phase: (A) 100 mM ammonium formate (pH 3.0, with formic acid); (B) water; (C) acetonitrile
	flow rate: 0.3 mL/min column temp.: 35 $^{\circ}$ C detector: ESI (+), full scan
	injection: 2 μ L
	sample: as indicated, in 10:90, (50 mM ammonium formate/formic acid, (pH 3.0):acetonitrile